




**Interlock™ -18 Fibered IDC™ Occlusion System**

<b>Standard Length 2D Configurations</b>						
<b>UPN</b>	<b>Description</b>	<b>Diameter (mm)</b>	<b>Length (cm)</b>	<b>Shape</b>		
M001361480	Interlock - 18 Coil	2	4	2D		
M001361490	Interlock - 18 Coil	2	6	2D		
M001361500	Interlock - 18 Coil	3	6	2D		
M001361510	Interlock - 18 Coil	3	12	2D		
M001361520	Interlock - 18 Coil	4	8	2D		
M001361530	Interlock - 18 Coil	4	15	2D		
M001361540	Interlock - 18 Coil	5	8	2D		
M001361550	Interlock - 18 Coil	5	15	2D		
M001361560	Interlock - 18 Coil	6	10	2D		
M001361570	Interlock - 18 Coil	6	20	2D		
M001361580	Interlock - 18 Coil	8	20	2D		
M001361590	Interlock - 18 Coil	10	20	2D		
M001361600	Interlock - 18 Coil	10	30	2D		
M001361610	Interlock - 18 Coil	12	20	2D		
M001361620	Interlock - 18 Coil	12	30	2D		
M001361630	Interlock - 18 Coil	14	20	2D		
M001361640	Interlock - 18 Coil	14	30	2D		
<b>Long Length 2D Configurations</b>						
<b>UPN</b>	<b>Description</b>	<b>Diameter (mm)</b>	<b>Length (cm)</b>	<b>Shape</b>		
M001361920	Interlock - 18 Coil	10	50	2D		
M001361930	Interlock - 18 Coil	14	50	2D		
M001361940	Interlock - 18 Coil	18	50	2D		
M001361950	Interlock - 18 Coil	20	50	2D		
M001361960	Interlock - 18 Coil	22	60	2D		
<b>Diamond Configurations</b>						
<b>UPN</b>	<b>Description</b>	<b>Diameter (mm)</b>	<b>Length (cm)</b>	<b>Shape</b>		
M001361740	Interlock - 18 Coil	2/3	2.3	Diamond		
M001361750	Interlock - 18 Coil	2/4	4.1	Diamond		
M001361760	Interlock - 18 Coil	2/5	5.8	Diamond		
M001361770	Interlock - 18 Coil	2/6	8	Diamond		

**Direxion Torqueable Microcatheter**

<b>UPN</b>	<b>Order Number</b>	<b>Usable Length (cm)</b>	<b>Tip Shape</b>	<b>RO Markers</b>
M001195320	19-532	130	Straight	2
M001195340	19-534	2	Bern	2

Illustrations are not necessary to scale. All images are property of Boston Scientific.

0.018-inch (0.457-mm)

Interlock and Fibered IDC are unregistered trademarks of Boston Scientific Corporation or its affiliates.

All cited trademarks are the property of their respective owners. CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for the use only in countries with applicable health authority product registrations.

PI-213401-AA JAN 2014 Printed in Germany by medicalvision.

**Boston Scientific**  
Advancing science for life™


www.bostonscientific-international.com

© 2013 Boston Scientific Corporation or its affiliates. All rights reserved. DINONC3503EA

**Boston Scientific**  
Advancing science for life™

**Interlock™ -18 Coil**  
Fibered IDC™ Occlusion System

*A little smaller and  
A lot Bigger*

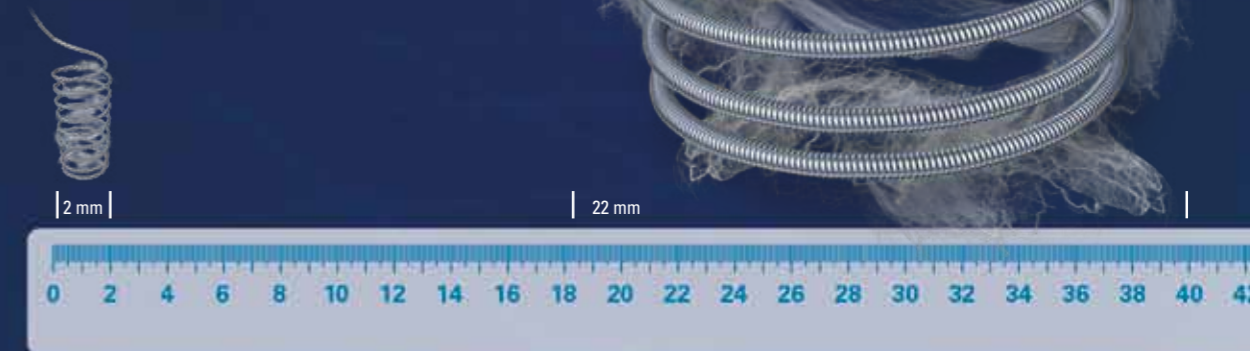


Images are not drawn to scale

# Lock In Accuracy, Power and Precision

In a prospective, randomized, single-center study, the use of the Interlock™ Fibered IDC™ Occlusion System for embolization of the GDA allowed investigators to place significantly fewer coils.

Number of Coils Used Per Procedure

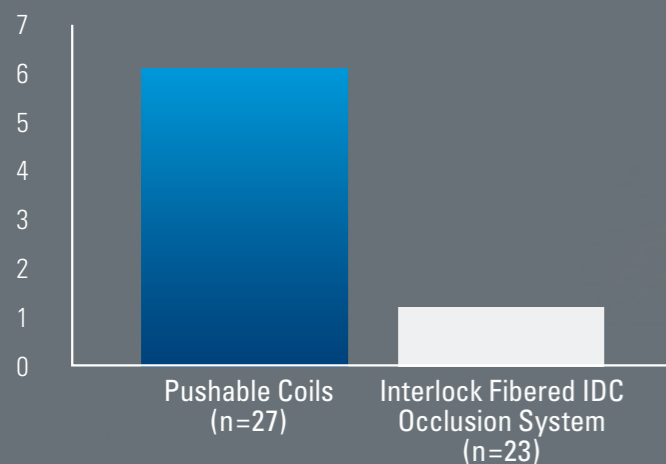

Dudek, et al, Embolization of the Gastroduodenal Artery Before Selective Internal Radiotherapy: A Prospectively Randomized Trial Comparing Standard Pushable Coils with Fibered Interlock Detachable Coils. CVIR, April 14, 2010.

- 83.6% of cases (19 of 23) achieved complete occlusion with one Interlock Fibered IDC Occlusion Coil.
- A shorter procedure time was observed for procedures utilizing detachable coils when compared to pushable coils.
- No coil migration was observed in the detachable coil group, whereas one incidence of migration was observed in the pushable coil group.

## Accuracy

Interlocking arms offer physicians the potential for greater control, precision and retractability.

## Precision\*


Broad range of product sizes including 2–22 mm diameters and up to 60 cm lengths.

## Power

Highly thrombogenic fibering configuration and long coil lengths engineered for fast and reliable vessel occlusion.

\* For placement accuracy and control in delivery you can now use Direxion™ torqueable microcatheter with Double Radiopaque Marker.

### Microcatheter with 1 Radiopaque marker

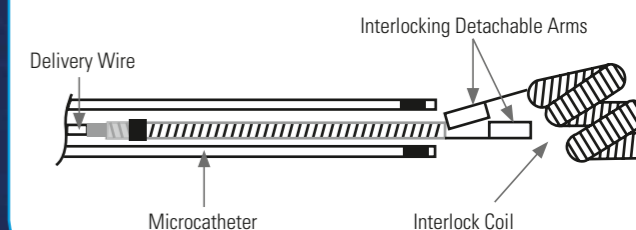

### Microcatheter Double Marker

